

S & N LABS

2021 E. Fourth Street

Santa Ana, California 92705

(714) 543-2211

27 September 2019

Job Number:	23437
PO Number:	verbal

Chemyo, LLC
4023 Kennett Pike, Suite 59371
Wilmington, Delaware 19807

REPORT OF ANALYSIS

One small plastic bag labeled "S4" was received on 23 September 2019. The powder in the bag was analyzed by Fourier-transform infrared spectroscopy (FT-IR) and matched reference standards of andarine (S4).

The powder was also analyzed for purity using high pressure liquid chromatography (HPLC). The results are summarized in the table below.

Sample	Purity at 210nm
S4	99.3

Neil E. Spingarn, Ph.D.
President

23437

S&N Labs

2021 E. Fourth Street, Suite 112
Santa Ana, CA 92705
Tel: 714-543-2211


Sample: S4 (No Lot Number)

Date: 09/23/2019

Analyst: Chris French

Client:

Chemyo LLC

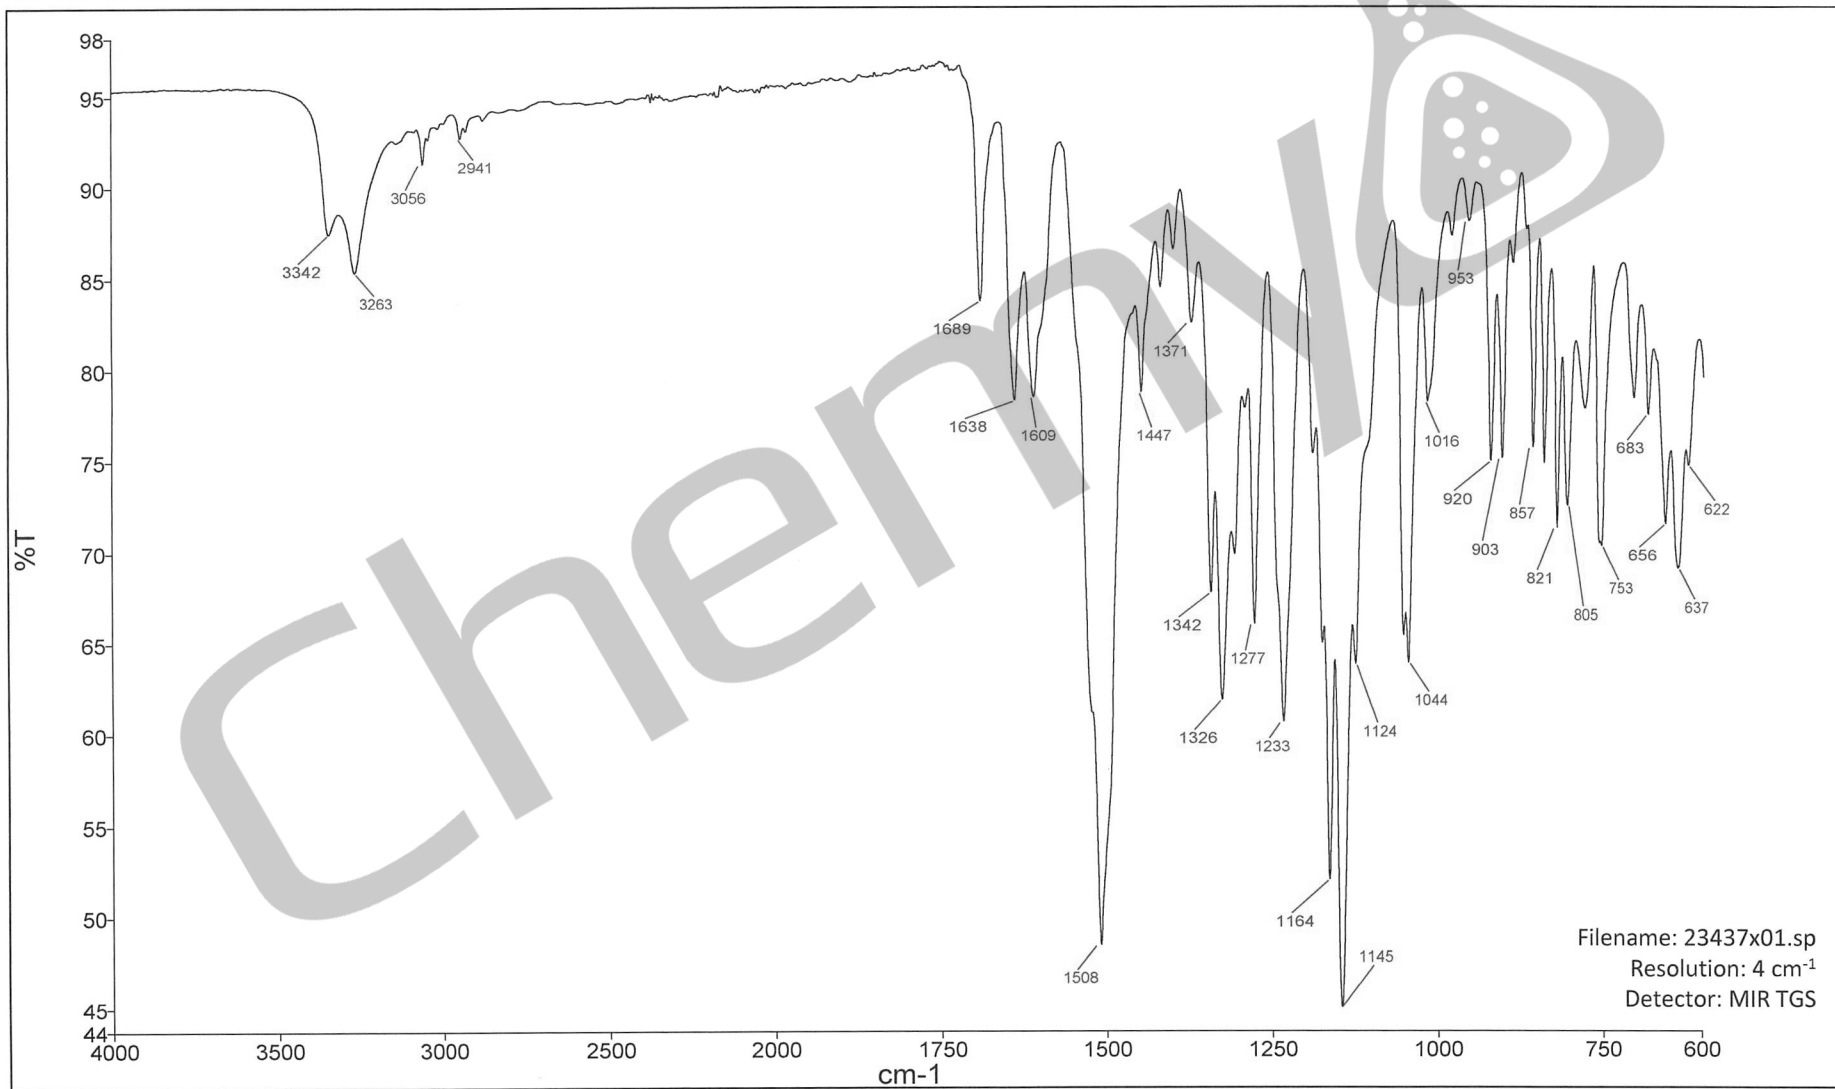


Chromatogram and Results

Injection Details

Injection Name:	23437 - S4 (40:1 dilution)	Run Time (min):	30.00
Vial Number:	A6	Injection Volume:	10.00
Injection Type:	Unknown	Channel:	UV_VIS_1
Calibration Level:		Wavelength:	210.0
Instrument Method:	23437 & 23439 - S4 & CB-03-01 purity	Bandwidth:	11
Processing Method:	23437 & 23439 - S4 & CB-03-01 purity	Dilution Factor:	1.0000
Injection Date/Time:	27/Sep/19 10:54	Sample Weight:	1.0000

Chromatogram

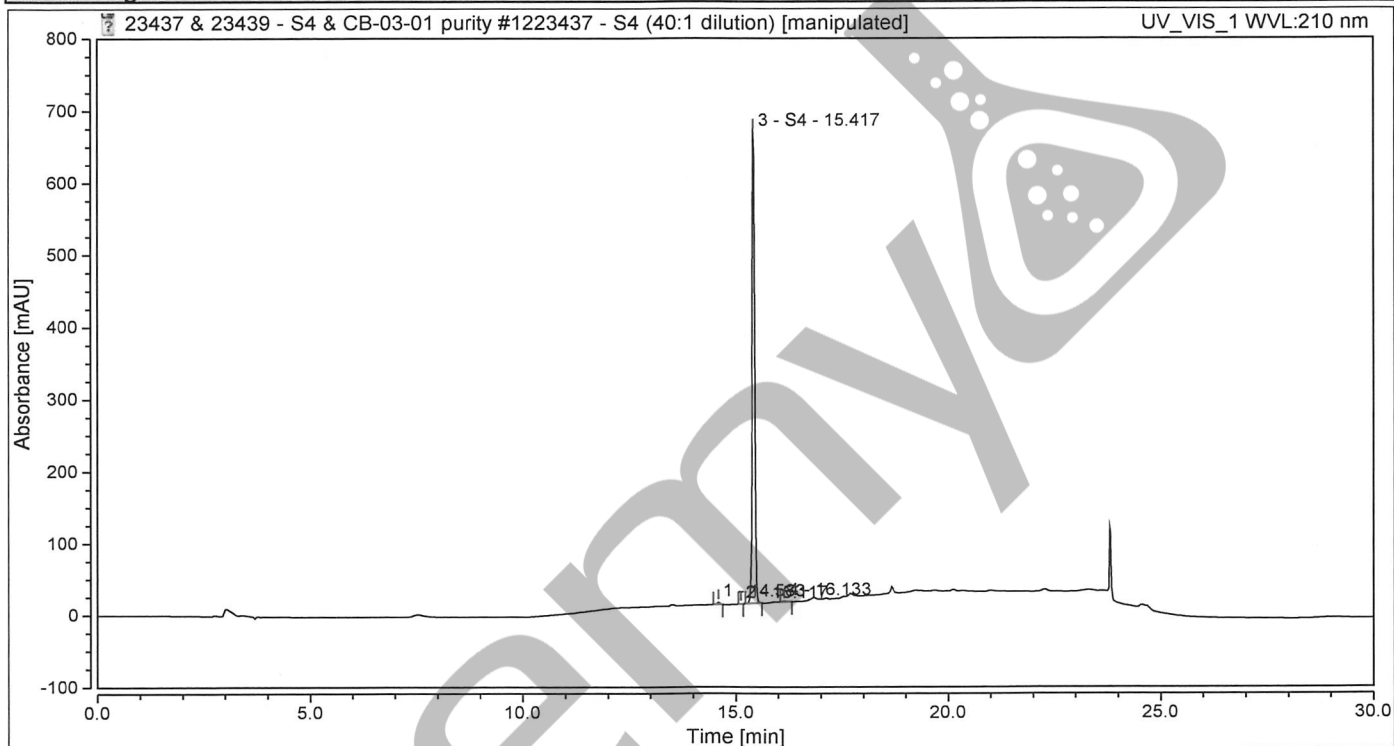

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount µg/ml
1		14.583	0.242	3.178	0.49	0.48	n.a.
2		15.117	0.025	0.418	0.05	0.06	n.a.
3	S4	15.417	48.691	654.711	99.28	99.29	n.a.
4		16.133	0.087	1.077	0.18	0.16	n.a.
n.a.	CB-03-01	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			49.045	659.384	100.00	100.00	